




Your complimentary  
use period has ended.  
Thank you for using  
PDF Complete.

[Click Here to upgrade to](#)

[Unlimited Pages and Expanded Features](#)

File: 0828\_multisizer\yFB86\_0uMGal\yFB86\_0uMGal\_1\_01.#M3  
Preference file: C:\MSI\Default.pri (modified)  
Group ID: yFB86\_0uMGal  
Sample ID: 1  
Run number: 1  
Electrolyte: ISOTON II  
Aperture diameter: 30  $\mu\text{m}$  Kd: 38.899  
Aperture current: 400  $\mu\text{A}$  Gain: 8  
Size bins: 300 from 0.6  $\mu\text{m}$  to 18  $\mu\text{m}$   
Sigma: 30,866 (Coincidence corrected)  
Count > 0.719  $\mu\text{m}$ : 30,000 Coincidence corrected: 30,866  
Coincidence correction: 2.9%  
Control mode: Total Count 30,000  
Elapsed time: 60.18 seconds  
Acquired: 19:39 28 Aug 2019  
Dilution Factor: 500  
Electrolyte volume: 10 mL

### Differential Number

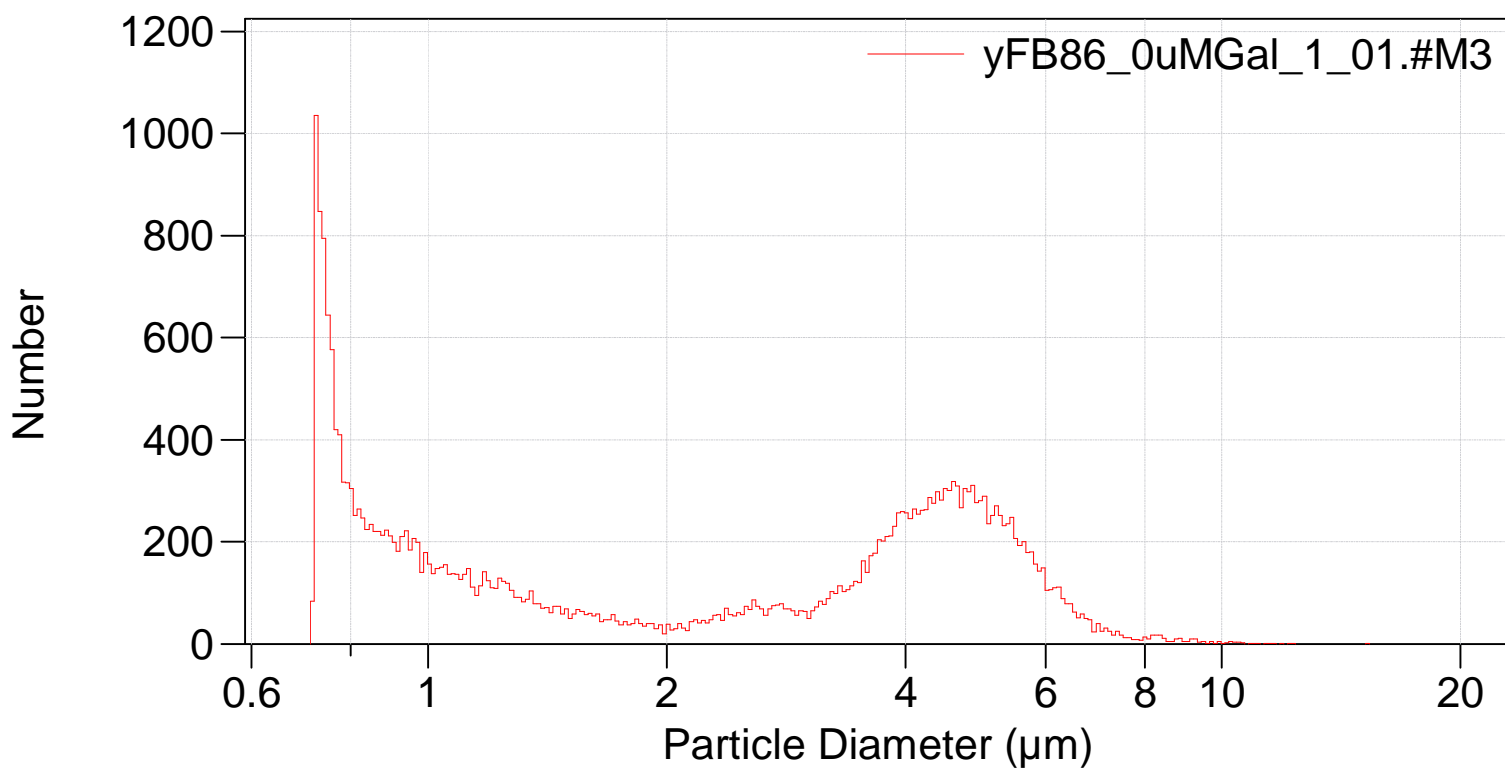

**Sigma = 30,866**